

**Quality ID #393: Infection within 180 Days of Cardiac Implantable Electronic Device (CIED)
Implantation, Replacement, or Revision**
– National Quality Strategy Domain: Patient Safety
– Meaningful Measure Area: Healthcare Associated Infections

2022 COLLECTION TYPE:
MIPS CLINICAL QUALITY MEASURES (CQMS)

MEASURE TYPE:
Outcome – High Priority

DESCRIPTION:
Infection rate following CIED device implantation, replacement, or revision.

INSTRUCTIONS:
This measure is to be submitted a minimum of **once per performance period** for patients with a CIED device implantation, replacement, or revision performed from January 1, 2021 through June 30, 2021 of the performance period. This measure may be submitted by Merit-based Incentive Payment System (MIPS) eligible clinicians who perform the quality actions described in the measure based on the services provided and the measure-specific denominator coding.

NOTE: *Include only patients that have had CIED implantation, replacement, or revision performed by **June 30, 2021**. This timeframe allows for evaluation of infection required within 180 days within the performance period. This will allow the evaluation of infection status post CIED implantation, replacement, or revision within the performance period.*

Infection rates for new implants shall be calculated and submitted separately from device replacements and revisions.

Additional submitting stratification categories may be useful; however, these stratifications are not required for purposes of QPP submission:

- Device class (e.g., pacemaker, ICD) and type (e.g., single chamber, dual chamber);
- Advanced renal disease (CKD stages 4 and 5, ESRD);
- Diabetes;
- CIED infection requiring device removal within 180 days prior to index CIED procedures; and
- CIED-related surgical procedure within 180 days prior to current CIED procedure.

Measure Submission Type:

Measure data may be submitted by individual MIPS eligible clinicians, groups, or third party intermediaries. The listed denominator criteria are used to identify the intended patient population. The numerator options included in this specification are used to submit the quality actions as allowed by the measure. The quality data codes listed do not need to be submitted by MIPS eligible clinicians, groups, or third party intermediaries that utilize this modality for submissions; however, these codes may be submitted for those third party intermediaries that utilize Medicare Part B claims data. For more information regarding Application Programming Interface (API), please refer to the Quality Payment Program (QPP) website.

THERE ARE TWO SUBMISSION CRITERIA FOR THIS MEASURE:

- 1) Patients, regardless of age, with a new CIED

OR

- 2) Patients, regardless of age, with a replaced or revised CIED

SUBMISSION CRITERIA 1: PATIENTS WITH A NEW CIED

DENOMINATOR (SUBMISSION CRITERIA 1):

All patients with a new CIED from January 1, 2021 through June 30, 2021 of the performance period

Definition:

CIEDs encompassed for this measure are the following devices:

- Pacemaker devices (single or dual chamber);
- Implantable cardioverter-defibrillators (ICDs, single or dual chamber);
- Cardiac resynchronization devices (pacemaker or ICD); and
- Implantable loop recorders (ILRs)

Denominator Criteria (Eligible Cases) 1:

All patients, regardless of age

AND

Procedure code for implantation, replacement, or revision of a CIED (ICD-10-PCS): 0JH604Z, 0JH605Z, 0JH606Z, 0JH607Z, 0JH608Z, 0JH609Z, 0JH60PZ, 0JH634Z, 0JH635Z, 0JH636Z, 0JH637Z, 0JH638Z, 0JH639Z, 0JH63PZ, 0JH804Z, 0JH805Z, 0JH806Z, 0JH807Z, 0JH808Z, 0JH809Z, 0JH80PZ, 0JH834Z, 0JH835Z, 0JH836Z, 0JH837Z, 0JH838Z, 0JH83PZ, 0JPT0PZ, 0JPT3PZ, 0JWT0PZ, 0JWT3PZ

WITHOUT

Telehealth Modifier: GQ, GT, 95, POS 02

AND/OR

Patient encounter during performance period (CPT): 33202, 33203, 33206, 33207, 33208, 33212, 33213, 33214, 33215, 33216, 33217, 33218, 33220, 33221, 33222, 33223, 33224, 33226, 33227, 33228, 33229, 33240, 33249, 33262, 33263, 33264, 33270

WITHOUT

Telehealth Modifier: GQ, GT, 95, POS 02

AND

New CIED

AND NOT

DENOMINATOR EXCLUSION:

Procedure code for heart transplantation (ICD-10-PCS): 02YA0Z0, 02YA0Z1, 02YA0Z2

NUMERATOR (SUBMISSION CRITERIA 1):

The number of patients from the denominator admitted with an infection requiring device removal or surgical revision within 180 days following CIED implantation, replacement, or revision

Numerator Instructions:

INVERSE MEASURE – A lower calculated performance rate for this measure indicates better clinical care or control. The “Performance Not Met” numerator option for this measure is the representation of the better clinical quality or control. Submitting that numerator option will produce a performance rate that trends closer to 0%, as quality increases. For inverse measures, a rate of 100% means all of the denominator eligible patients did not receive the appropriate care or were not in proper control.

Numerator Options:

Performance Met:

Patient admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision (**G9410**)

OR

Performance Not Met:

Patient not admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision (**G9411**)

OR

SUBMISSION CRITERIA 2: PATIENTS WITH A REPLACED OR REVISED CIED

DENOMINATOR (SUBMISSION CRITERIA 2):

All patients with replacement or revision of a CIED from January 1, 2021 through June 30, 2021 of the performance period

Definition:

CIEDs encompassed for this measure are the following devices:

- Pacemaker devices (single or dual chamber);
- Implantable cardioverter-defibrillators (ICDs, single or dual chamber);
- Cardiac resynchronization devices (pacemaker or ICD); and
- Implantable loop recorders (ILRs)

Denominator Criteria (Eligible Cases) 2:

All patients, regardless of age

AND

Procedure code for implantation, replacement, or revision of a CIED (ICD-10-PCS): 0JH604Z, 0JH605Z, 0JH606Z, 0JH607Z, 0JH608Z, 0JH609Z, 0JH60PZ, 0JH634Z, 0JH635Z, 0JH636Z, 0JH637Z, 0JH638Z, 0JH639Z, 0JH63PZ, 0JH804Z, 0JH805Z, 0JH806Z, 0JH807Z, 0JH808Z, 0JH809Z, 0JH80PZ, 0JH834Z, 0JH835Z, 0JH836Z, 0JH837Z, 0JH838Z, 0JH83PZ, 0JPT0PZ, 0JPT3PZ, 0JWT0PZ, 0JWT3PZ

WITHOUT

Telehealth Modifier: GQ, GT, 95, POS 02

AND/OR

Patient encounter during performance period (CPT): 33202, 33203, 33206, 33207, 33208, 33212, 33213, 33214, 33215, 33216, 33217, 33218, 33220, 33221, 33222, 33223, 33224, 33226, 33227, 33228, 33229, 33240, 33249, 33262, 33263, 33264, 33270

WITHOUT

Telehealth Modifier: GQ, GT, 95, POS 02

AND

Replaced or revised CIED

AND NOT

DENOMINATOR EXCLUSION:

Procedure code for heart transplantation (ICD-10-PCS): 02YA0Z0, 02YA0Z1, 02YA0Z2

NUMERATOR (SUBMISSION CRITERIA 2):

The number of patients from the denominator admitted with an infection requiring device removal or surgical revision within 180 days following CIED implantation, replacement, or revision.

Numerator Instructions:

INVERSE MEASURE – A lower calculated performance rate for this measure indicates better clinical care or control. The “Performance Not Met” numerator option for this measure is the representation of the better clinical quality or control. Submitting that numerator option will produce a performance rate that trends closer to 0%, as quality increases. For inverse measures, a rate of 100% means all of the denominator eligible patients did not receive the appropriate care or were not in proper control.

Numerator Options:

Performance Met:

Patient admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision (**G9412**)

OR

Performance Not Met:

Patient not admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision (**G9413**)

RATIONALE:

The rate of implantable cardioverter-defibrillator (ICD) infections has been increasing faster than that of device implantation and is associated with substantial morbidity, mortality, and financial cost. A recent study including over 200,000 ICD implant patients found 2 percent of patients undergoing ICD implantation experienced a device-related infection. Patients who developed an ICD infection were likely to have more comorbidity burden, warfarin use, coronary sinus lead, device upgrade/malfunction as the last surgery, peri-ICD implant complications, and non-EP trained operator. The evidence demonstrates the need to measure performance in this area.

CLINICAL RECOMMENDATION STATEMENTS:

In recognition that there is an absence of applicable physician-level performance measures for the profession of cardiac electrophysiology, the Heart Rhythm Society (the international professional society focused on the care of patients with heart rhythm disorders) convened a Performance Measures Development Task Force to consider and develop potential physician-level measures for cardiac electrophysiologists. The task force consisted of thought leaders in 1) implantation of cardiac implantable electronic devices (CIEDs) including pacemakers, implantable cardioverter defibrillators (ICDs), cardiac resynchronization devices (pacemaker or ICD), and implantable loop recorders (ILRs); 2) cardiovascular health policy; 3) performance measures development; 4) clinical outcomes; and 5) population science.

The process for consideration of the evidence included review of the relevant literature referenced within this document and in the knowledge of the members of the task force (Voigt et al, 2006; Cabell et al, 2004; Voigt et al, 2010; Greenspon et al, 2011; Sohail et al, 2011; Nery et al, 2010; Ferguson et al, 1996; Uslan et al, 2007; Lee et al, 2010; Klug et al, 2007; Alter et al, 2005; Al-Khatib et al, 2008; de Oliveira et al, 2009; Uslan et al, 2011; Borleffs et al, 2010; Sohail et al, 2007; Bloom et al, 2006; Baddour et al, 2010; Le KY et al, 2011; Johansen et al, 2011; Al-Khatib et al, 2005; Tarakji et al, 2010).

The number of CIED-related infections in the United States continues to increase out of proportion to the increase in the CIED implantation rates (Voigt et al, 2006; Cabell et al, 2004; Voigt et al, 2010). This infection burden is associated with increased mortality, prolonged hospital stays, and high financial costs (Greenspon et al, 2011; Sohail et al, 2011; Ferguson et al, 1996). Collectively, the incidence of CIED infection has ranged from 0.3 to 2.9% across the literature evaluated (Greenspon et al, 2011; Sohail et al, 2011; Nery et al, 2010; Uslan et al, 2007; Lee et al, 2010; Klug et al, 2007; Alter et al, 2005; Al-Khatib et al, 2008; Uslan et al, 2011; Bloom et al, 2006; Baddour et al, 2010; Johansen et al, 2011). In the vast majority of patients, CIED infection is preventable, and an association between a higher volume of ICD implants and a lower rate of infections has been demonstrated (Tarakji et al, 2010). This is why a performance measure that could lower the risk of CIED infection is critically needed.

COPYRIGHT:

© American College of Cardiology Foundation, 2021. All rights reserved. CPT® contained in the Measure specifications is copyright 2004-2021


American Medical Association. LOINC® copyright 2004-2021 Regenstrief Institute, Inc.

This material contains SNOMED Clinical Terms® (SNOMED CT®) copyright 2004-2021 International Health Terminology Standards Development Organisation.


ICD-10 is copyright 2021 World Health Organization. All Rights Reserved.

**2022 Clinical Quality Measure Flow for Quality ID #393:
Infection Within 180 Days of Cardiac Implantable Electronic Device (CIED)
Implantation, Replacement, or Revision
Submission Criteria 1****

Disclaimer: Refer to the measure specification for specific coding and instructions to submit this measure.

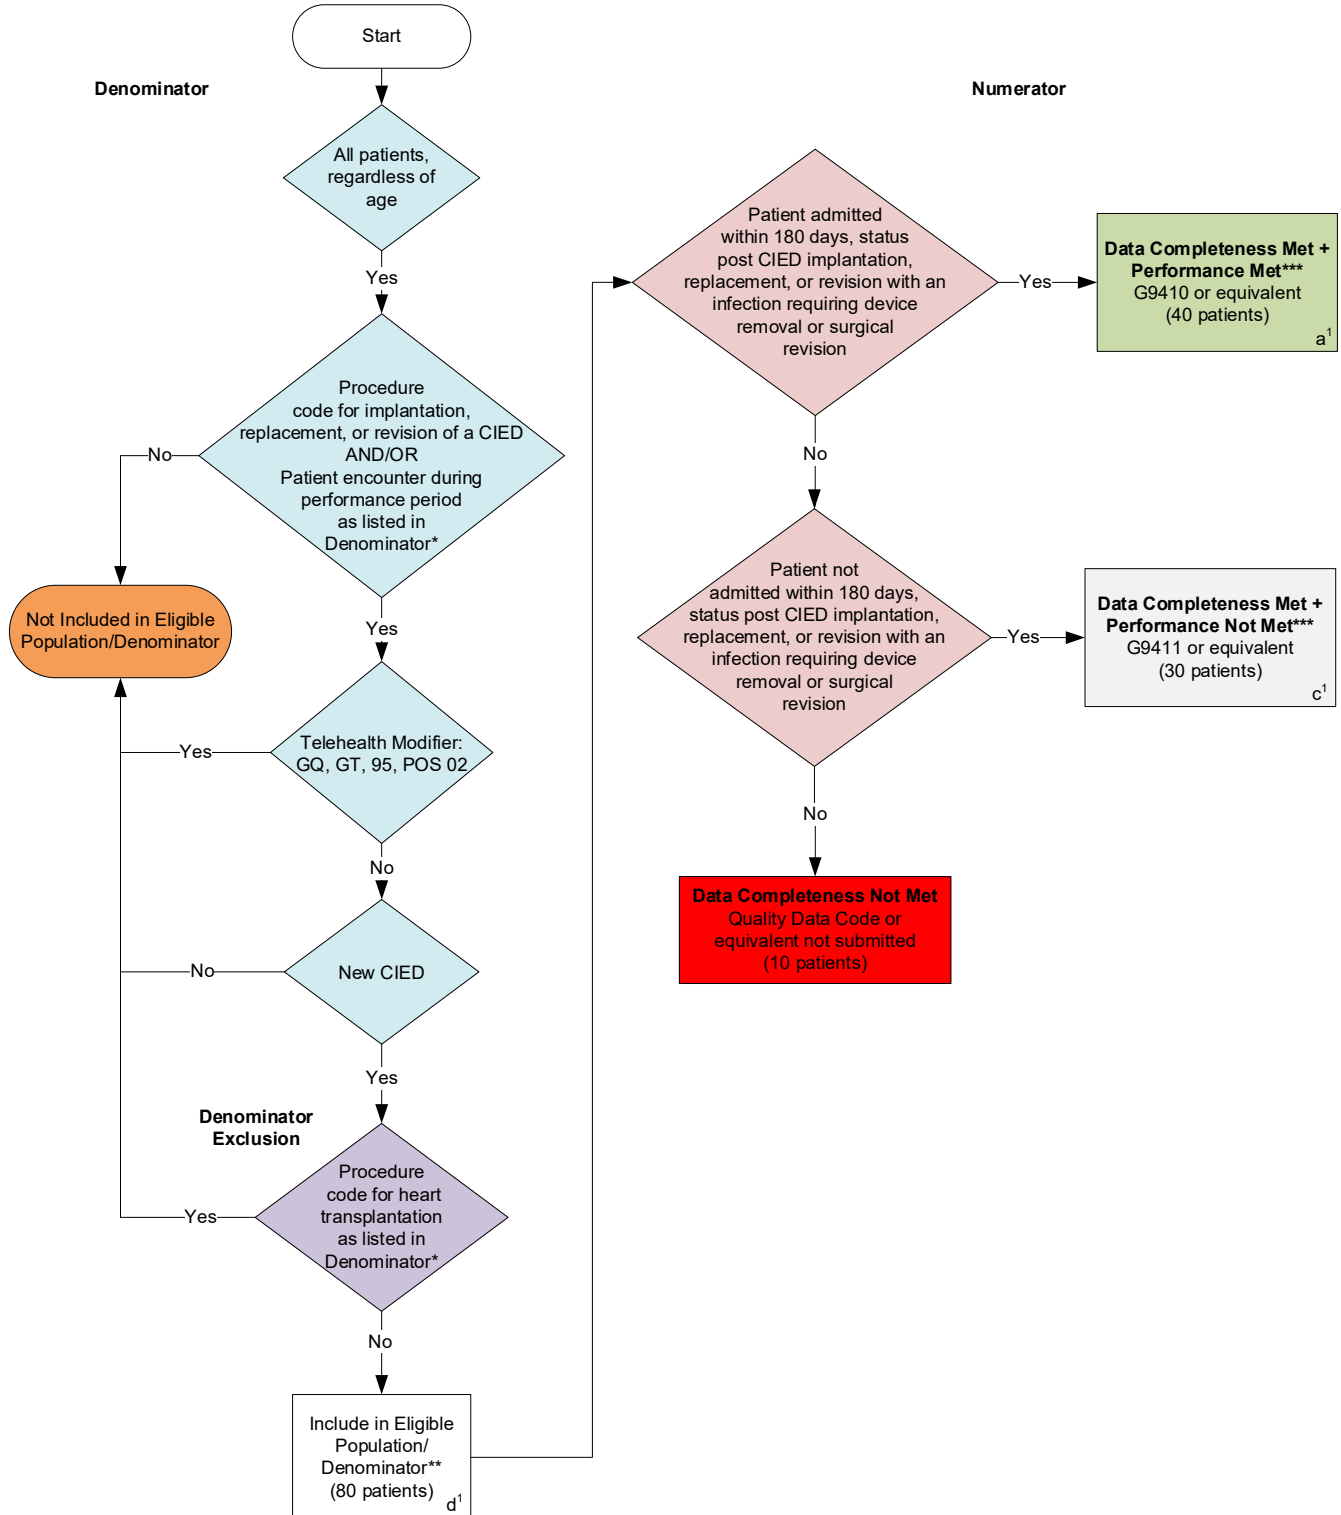

Submission Criteria 2**

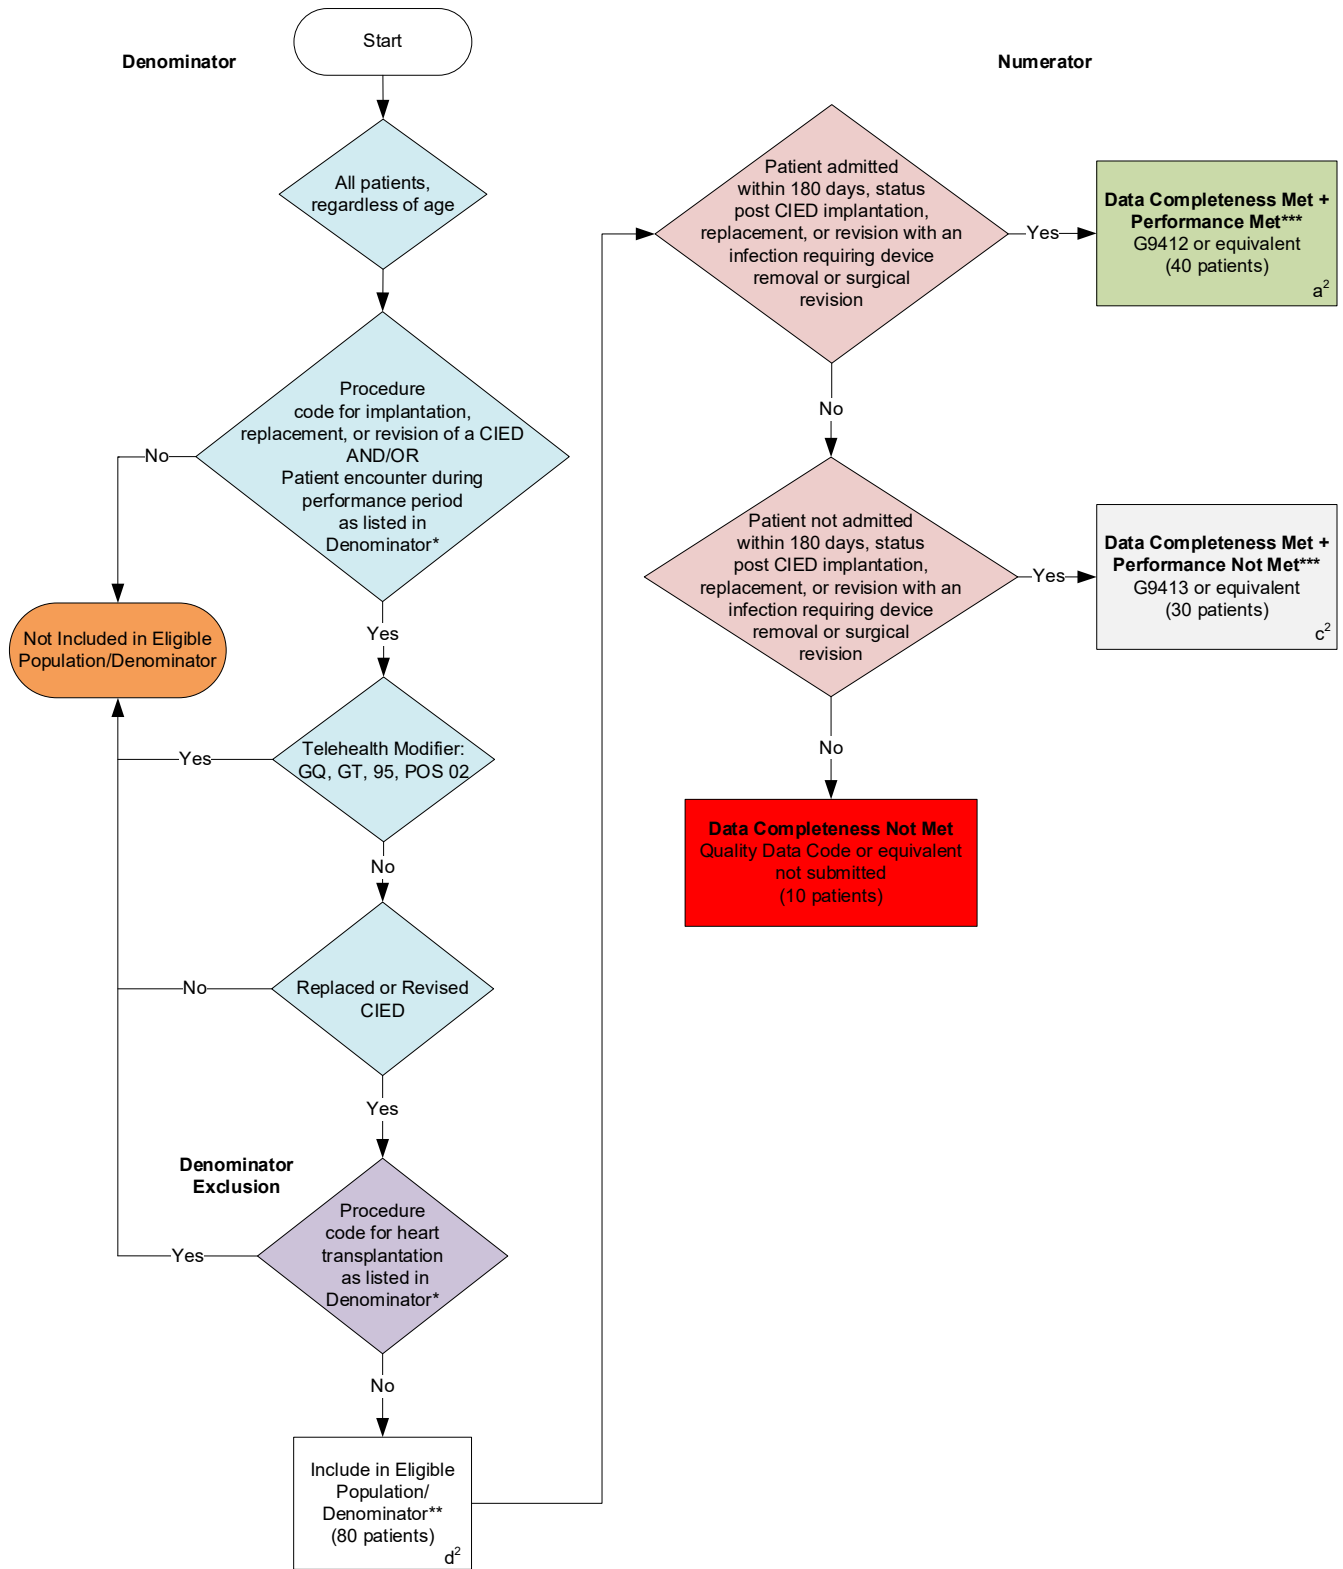

SAMPLE CALCULATIONS

Data Completeness=

$$\frac{\text{Performance Met (a}^1\text{+a}^2\text{=80 patients)} + \text{Performance Not Met (c}^1\text{+c}^2\text{=60 patients)}}{\text{Eligible Population / Denominator (d}^1\text{+d}^2\text{=160 patients)}} = \frac{140 \text{ patients}}{160 \text{ patients}} = 87.50\%$$

Performance Rate=

$$\frac{\text{Performance Met (a}^1\text{+a}^2\text{=80 patients)}}{\text{Data Completeness Numerator (140 patients)}} = \frac{80 \text{ patients}}{140 \text{ patients}} = 57.14\%$$

*See the posted measure specification for specific coding and instructions to submit this measure.

This measure flow illustrates denominator eligible encounters as requiring a ICD-10-PCS AND/OR an encounter.

The measurement period is for patients with a CIED device implantation, replacement, or revision performed from January 1, 2021 through June 30, 2021 of the performance period.

**This measure has two Submission Criteria that are combined for calculation of one data completeness and one performance rate.

***A lower calculated performance rate for this measure indicates better clinical care or control.

NOTE: Submission Frequency: Patient-Process

CPT only copyright 2021 American Medical Association. All rights reserved.
The measure diagrams were developed by CMS as a supplemental resource to be used in conjunction with the measure specifications. They should not be used alone or as a substitution for the measure specification.

v6

**2022 Clinical Quality Measure Flow Narrative for Quality ID #393:
Infection Within 180 Days of Cardiac Implantable Electronic Device (CIED)
Implantation, Replacement, or Revision**

Disclaimer: Refer to the measure specification for specific coding and instructions to submit this measure.

Submission Criteria One:

1. Start with Denominator
2. *All patients, regardless of age*
3. Check *Procedure code for implantation, replacement, or revision of a CIED AND/OR Patient encounter during performance period as listed in Denominator**:
 - a. *If Procedure code for implantation, replacement, or revision of a CIED AND/OR Patient encounter during performance period as listed in Denominator* equals No, do not include in Eligible Population/Denominator. Stop processing.*
 - b. *If Procedure code for implantation, replacement, or revision of a CIED AND/OR Patient encounter during performance period as listed in Denominator* equals Yes, proceed to check Telehealth Modifier.*
4. Check *Telehealth Modifier*:
 - a. *If Telehealth Modifier equals Yes, do not include in Eligible Population/Denominator. Stop processing.*
 - b. *If Telehealth Modifier equals No, proceed to check New CIED.*
5. Check *New CIED*:
 - a. *If New CIED equals No, do not include in Eligible Population/Denominator. Stop processing.*
 - b. *If New CIED equals Yes, proceed to check Procedure code for heart transplantation as listed in Denominator*.*
6. Check *Procedure code for heart transplantation as listed in Denominator**:
 - a. *If Procedure code for heart transplantation as listed in Denominator* equals Yes, do not include in Eligible Population/Denominator. Stop processing.*
 - b. *If Procedure code for heart transplantation as listed in Denominator* equals No, include in Eligible Population/Denominator.*
7. Denominator Population:
 - Denominator Population is all Eligible Patients in the Denominator. Denominator is represented as Denominator in the Sample Calculation listed at the end of this document. Letter d¹ equals 80 patients in the Sample Calculation.
8. Start Numerator
9. Check *Patient admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision*:
 - a. *If Patient admitted within 180 days, status post CIED implantation, replacement, or revision with an*

infection requiring device removal or surgical revision equals Yes, include in Data Completeness Met and Performance Met.

- *Data Completeness Met and Performance Met* letter is represented in the Data Completeness and Performance Rate in the Sample Calculation listed at the end of this document. Letter a¹ equals 40 patients in the Sample Calculation.
- b. *If Patient admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision equals No, proceed to check Patient not admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision.*
10. Check *Patient not admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision*:
- a. *If Patient not admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision equals Yes, include in Data Completeness Met and Performance Not Met.*
- *Data Completeness Met and Performance Not Met* letter is represented in the Data Completeness in the Sample Calculation listed at the end of this document. Letter c¹ equals 30 patients in the Sample Calculation.
- b. *If Patient Not Admitted within 180 days, Status Post CIED Implantation, Replacement, or Revision with an Infection Requiring Device Removal or Surgical Revision equals No, proceed to check Data Completeness Not Met.*
11. Check *Data Completeness Not Met*:
- *If Data Completeness Not Met, the Quality Data Code or equivalent was not submitted. 10 patients have been subtracted from the Data Completeness Numerator in the Sample Calculation.*

Submission Criteria Two:

1. Start with Denominator
2. *All patients, regardless of age*
3. Check *Procedure code for implantation, replacement, or revision of a CIED AND/OR Patient encounter during performance period as listed in Denominator**:
 - a. *If Procedure code for implantation, replacement, or revision of a CIED AND/OR Patient encounter during performance period as listed in Denominator* equals No, do not include in Eligible Population/Denominator. Stop processing.*
 - b. *If Procedure code for implantation, replacement, or revision of a CIED AND/OR Patient encounter during performance period as listed in Denominator* equals Yes, proceed to check Telehealth Modifier.*
4. Check *Telehealth Modifier*:
 - a. *If Telehealth Modifier equals Yes, do not include in Eligible Population/Denominator. Stop processing.*

- b. If *Telehealth Modifier* equals No, proceed to check *Replaced or Revised CIED*.
5. Check *Replaced or Revised CIED*:
 - a. If *Replaced or Revised CIED* equals No, do not include in *Eligible Population/Denominator*. Stop processing.
 - b. If *Replaced or Revised CIED* equals Yes, proceed to check *Procedure code for heart transplantation as listed in Denominator**.
6. Check *Procedure code for heart transplantation as listed in Denominator**:
 - a. If *Procedure code for heart transplantation as listed in Denominator** equals Yes, do not include in *Eligible Population/Denominator*. Stop processing.
 - b. If *Procedure code for heart transplantation as listed in Denominator** equals No, include in *Eligible Population/Denominator*.
7. Denominator Population:
 - Denominator Population is all Eligible Patients in the Denominator. Denominator is represented as Denominator in the Sample Calculation listed at the end of this document. Letter d² equals 80 patients in the Sample Calculation.
8. Start Numerator
9. Check *Patient admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision*:
 - a. If *Patient admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision* equals Yes, include in *Data Completeness Met and Performance Met*.
 - *Data Completeness Met and Performance Met* letter is represented in the Data Completeness and Performance Rate in the Sample Calculation listed at the end of this document. Letter a² equals 40 patients in the Sample Calculation.
 - b. If *Patient admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision* equals No, proceed to check *Patient not admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision*.
10. Check *Patient not admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision*:
 - a. If *Patient not admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision* equals Yes, include in *Data Completeness Met and Performance Not Met*.
 - *Data Completeness Met and Performance Not Met* letter is represented in the Data Completeness in the Sample Calculation listed at the end of this document. Letter c² equals 30 patients in the Sample Calculation.
 - b. If *Patient not admitted within 180 days, status post CIED implantation, replacement, or revision with an infection requiring device removal or surgical revision* equals No, proceed to check *Data Completeness Not Met*.

11. Check *Data Completeness Not Met*:

- If *Data Completeness Not Met*, the Quality Data Code or equivalent was not submitted. 10 patients have been subtracted from the Data Completeness Numerator in the Sample Calculation.

Sample Calculations

Data Completeness equals Performance Met (a^1 plus a^2 equals 80 patients) plus Performance Not Met (c^1 plus c^2 equals 60 patients) divided by Eligible Population / Denominator (d^1 plus d^2 equals 160 patients). All equals 140 patients divided by 160 patients. All equals 87.50 percent.

Performance Rate equals Performance Met (a^1 plus a^2 equals 80 patients) divided by Data Completeness Numerator (140 patients). All equals 80 patients divided by 140 patients. All equals 57.14 percent.

*See the posted measure specification for specific coding and instructions to submit this measure.

This measure flow illustrates denominator eligible encounters as requiring a ICD-10-PCS AND/OR an encounter.

The measurement period is for patients with a CIED device implantation, replacement, or revision performed from January 1, 2021 through June 30, 2021 of the performance period.

**This measure has two Submission Criteria that are combined for calculation of one data completeness and one performance rate.

***A lower calculated performance rate for this measure indicates better clinical care or control.

NOTE: Submission Frequency: Patient-Process

The measure diagrams were developed by CMS as a supplemental resource to be used in conjunction with the measure specifications. They should not be used alone or as a substitution for the measure specification.